
INDEPENDENTLY TESTED

RANKED No.1 FOR ACCURACY

Among four horizontal scan body systems tested in a newly published *in-vitro* study.

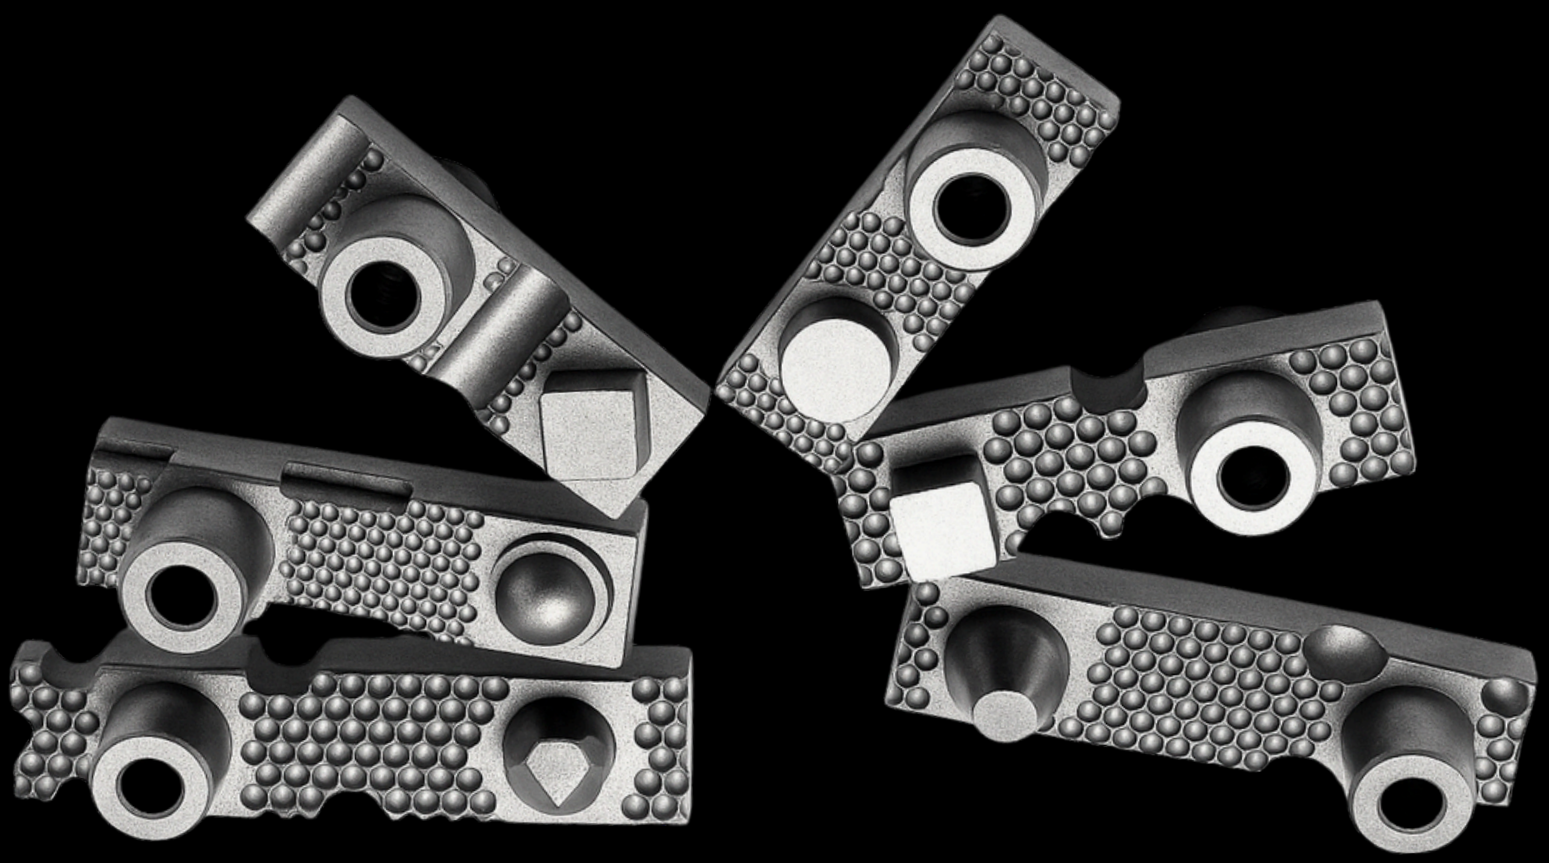

18.42 µm
LOWEST MEAN DEVIATION*

97.47 %
WITHIN 50 µm*

0.03 %
OVER 100 µm*

INDEPENDENT. PEER-REVIEWED. PRESSURE-TESTED.

GEOMETRY WINS.

ScanLadder

* Among the four horizontal scan-body systems evaluated in the study.